

EU-Type Examination - Production Type Certificate

This is to certify that:

Perry Baromedical Corporation
3750 Prospect Avenue
Riviera Beach
Florida
33404
USA

Holds Certificate Number:

CE 512611

In respect of:


Monoplace Hyperbaric Chambers - SIGMA 34, SIGMA 36 and SIGMA 40.

On the basis of our examination under the requirements of Council Directive 2014/68/EU Module B of the Pressure Equipment Directive, as transposed into the law of The Netherlands Warenwetbesluit drukapparatuur 2016.

For and on behalf of BSI, a Notified
Body for the above Directive
(Notified Body Number 2797):

Previous Notified Body: BSI 0086

First Issued: 2007-09-04



Drs. Dave Hagenaaars, Managing Director

Latest Issue: 2019-10-24

Expiry Date: 2027-09-03

EU-Type Examination - Production Type Certificate

No. CE 512611

Additional Information

Limitations of Certificate Validity

Monoplace Hyperbaric Chambers

Model Nos. SIGMA 34, SIGMA 36 and SIGMA 40


Technical File Ref. No. TECH-903638 Rev. F

PS = 2.34 bar g

TS = 0°C to 38°C

Fluid Groups 1 and 2 (Oxygen Rich Compressed Air)

Main Materials of Construction – Acrylic Window, Aluminium and Stainless/Carbon Steels

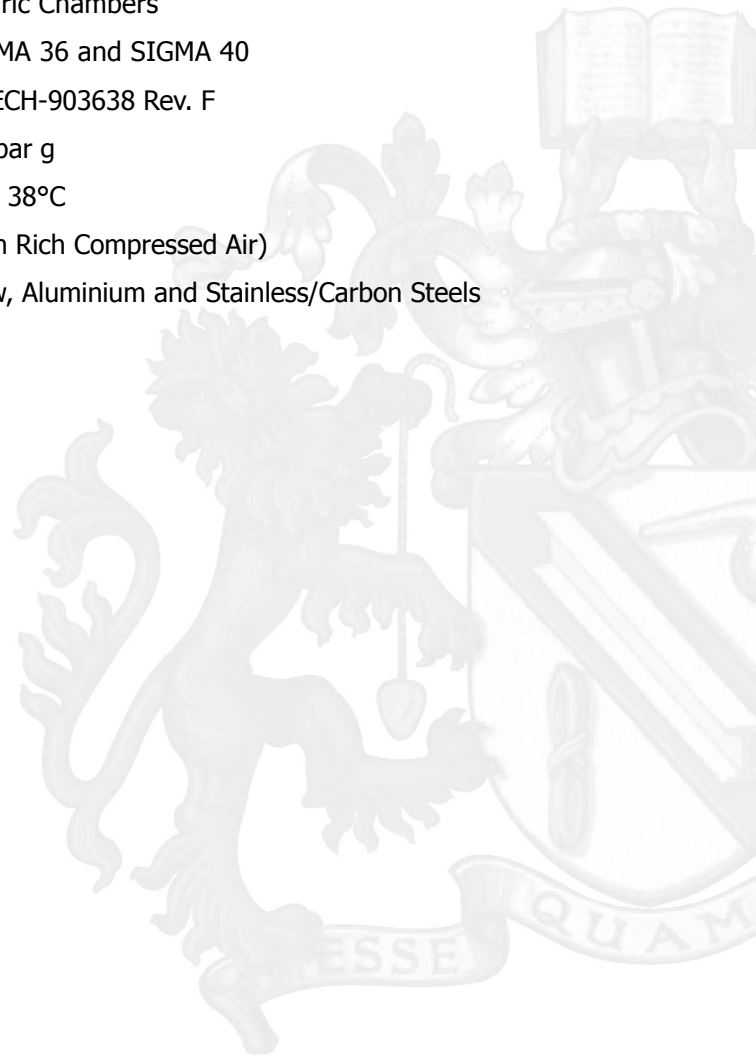

First Issued: 2007-09-04

Latest Issue: 2019-10-24

Expiry Date: 2027-09-03

Page: 2 of 2

This certificate has been issued by and remains the property of BSI Group The Netherlands B.V., John M. Keynesplein 9, 1066 EP Amsterdam, The Netherlands and should be returned immediately upon request.
To check its validity telephone +31 20 3460780. An electronic certificate can be authenticated [online](#).

BSI Group The Netherlands B.V., registered in the Netherlands under number 33264284, at John M. Keynesplein 9, 1066 EP Amsterdam, The Netherlands
A member of BSI Group of Companies.